



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Alpagas Sutton Inc./Francine Bédard
1474 Chemin Macey
Sutton QC J0E 2K0 Canada

08/09/13

Test No: 465382


Animal and Sample Description

Animal Name: Aztec Avagadro
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Rose Grey

Animal ID: 839749
Sample Location: Blanket
Sample Date: 05/17/13
Age: 06/25/02

Laboratory Data

Mean Fiber Diameter: 25.6 microns
Standard Deviation: 5.3 microns
Coefficient of Variation: 20.6 %
Fibers Greater Than 30 microns: 14.8 %

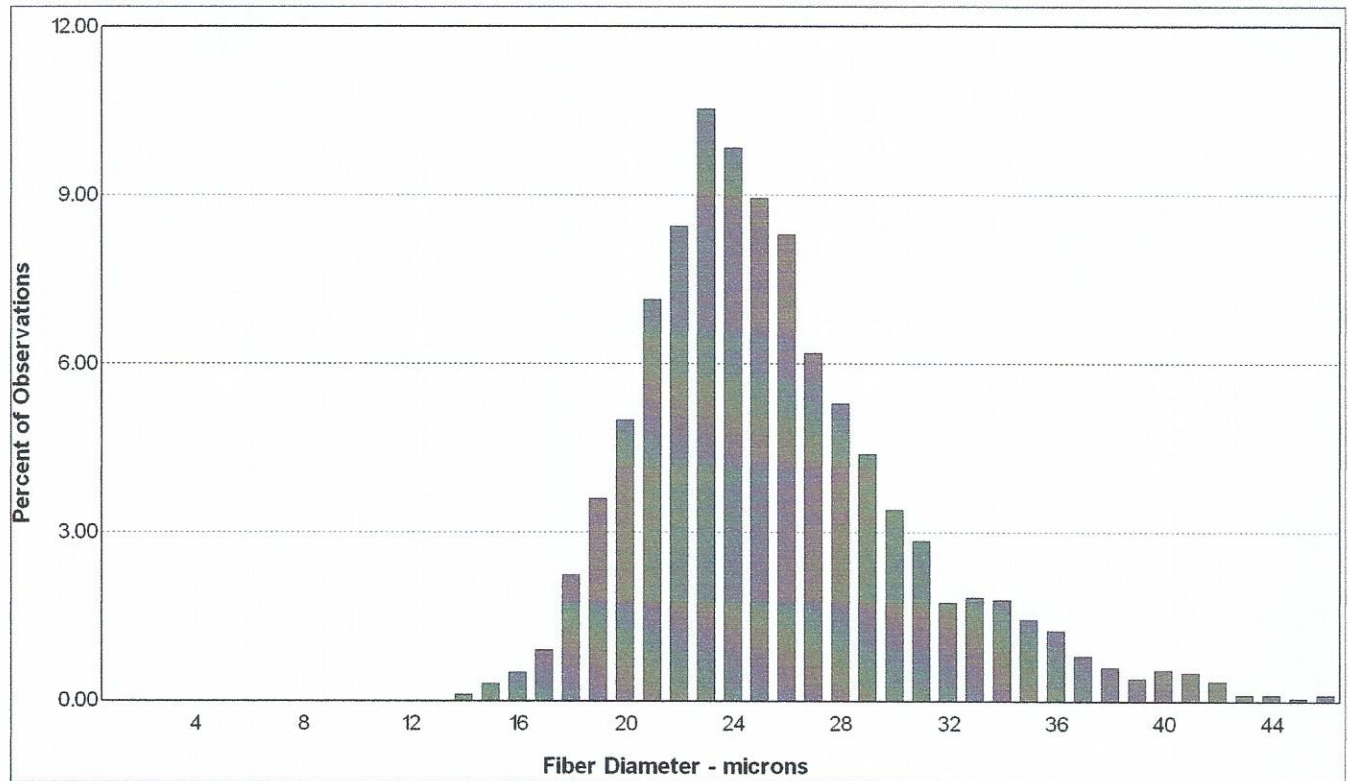

This Test Performed According to I.W.T.O Method 12